ROSE MOBILE™ REFERENCE GUIDE

DEVICE OVERVIEW

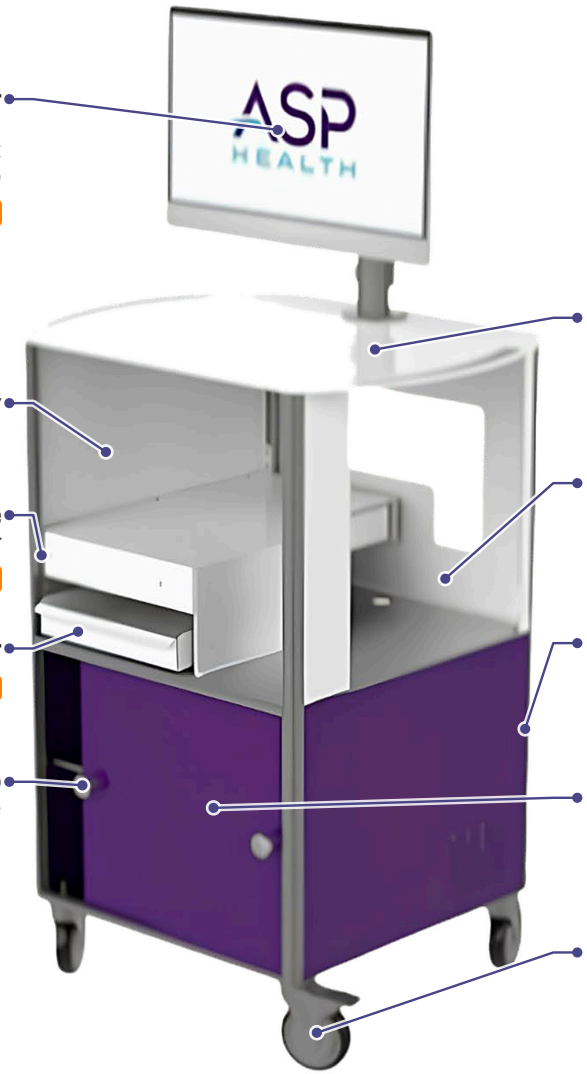

Monitor
On a VESA post; curved monitor max 22 lb
MAX 26 LB

Work Surface
Keyboard and mouse

ROSE View Bay
Left recessed area

ROSE Prep Bay
Feet sit in the pucks

Pull-Out Surface
Flips over to a drawer
MAX 10 LB

Front Drawer
MAX 10 LB

Computer & Power Strip
Lower rear bay

Cord Wrap
Left side

Storage Cabinet
Two shelves
UPPER SHELF MAX 10 LB

Locking Wheels
Colored wheel locks to roll straight

WARNING Do not exceed the tagged load limits.

QUICK SETUP

1 Position the cart

Stable, level floor indoors, away from direct sunlight and the sterile field. Keep 6 in clear at the front and right; leave the rear accessible.

2 Load the devices

ROSE View in the recessed bay on the left. ROSE Prep feet into the pucks on the right.

3 Add monitor and computer

Mount the monitor on the post; keyboard and mouse on top. The computer goes in the lower rear bay.

4 Connect the cords

Plug every device and computer cord into the power strip, routing cords through the grommets.

5 Power on

Unwrap the strip cord and plug it into the wall. Switch the power strip ON, then each device, then the computer.

TIP Larger computer tower? The lower-rear half wall swings open. See Setup in the User Manual.

WARNING

Electric shock hazard. Use only the supplied power strip and plug. Do not open or disassemble the cart. Keep wet hands off the power strip, and unplug by the plug, never the cord.

ROSE Mobile is non-medical equipment: a movable support surface and storage area for compatible equipment such as ROSE Prep™, ROSE View™, a computer and a monitor. It performs no clinical, diagnostic, therapeutic, analytical or device-control function. For indoor use by trained professionals in a clinic or laboratory. This quick reference guide is for reference purposes only. Please refer to the User Manual for complete information.

ROSE MOBILE™ REFERENCE GUIDE

EVERYDAY USE

Shut Down

Whenever the cart is not in use

1. Switch off each device and the computer.
2. Switch off the power strip.
3. Unplug the cord and wrap it on the cord wrap.

Move the Cart

Before moving it anywhere

1. Close all doors, trays and work surfaces.
2. Unlock the wheels; steer with the side handles.
3. Lock the wheels once the cart is in place.

TIP The colored wheel locks to roll in a straight line.

Clean

Between patients, and every day
Takes under 3 minutes

1. Switch the power off and put on gloves.
2. Use a soft 70% alcohol or germicidal wipe.
3. Decontaminate before storing over a week.

CAUTION No bleach-based wipes or harsh disinfectants or solvents.

WARNING Move with care over bumps and uneven floors, and don't drop devices or equipment. Never stand, sit or lean on the cart.

TROUBLESHOOTING



Power strip won't turn on

1. Unplug the power cord and plug it back in firmly.
2. Switch the power strip off, then on again.

Wheels are stiff or won't lock

1. Clear any debris caught in the wheels.
2. Still stiff? Contact ASP Health support.

Drawer, doors or pull-out surface stick

1. Clear any debris from the rail tracks.
2. Spray the tracks with WD-40 or a similar lubricant.
3. Still sticking? Contact ASP Health support.

Parts damaged, loose or missing

1. If the housing or electrical parts are damaged, do not use the cart.
2. Contact ASP Health support for replacement parts.

NOTE Problem not listed, or still not working? Contact ASP Health support and refer to the User Manual.